




Certificate of Analysis (CoA)

Product:	BPC157 & TB500
Quantity:	5 mg / 5 mg
Batch/Lot No.:	BT5-03-814-n086
Date of Analysis:	14 July 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

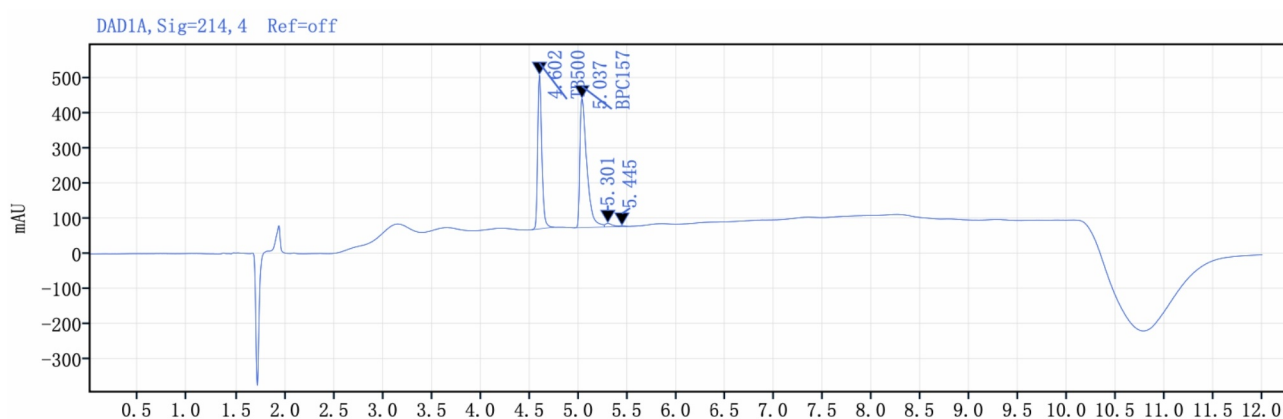

Quality Control

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	White to off-white lyophilized powder	White to off-white lyophilized powder (conforms)
Identification (Retention Time)	HPLC	±0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	≥ 99.0%	99.03%
Net Peptide Quantity	HPLC	5 mg / 5 mg	5.83 mg / 6.04 mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by: Matt C.
Matt C.
Head of Quality Control