




Certificate of Analysis (CoA)

Product:	GHK-Cu
Quantity:	50mg
Batch/Lot No.:	GK50-01-905-g387
Date of Analysis:	20 Nov 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

Quality Control

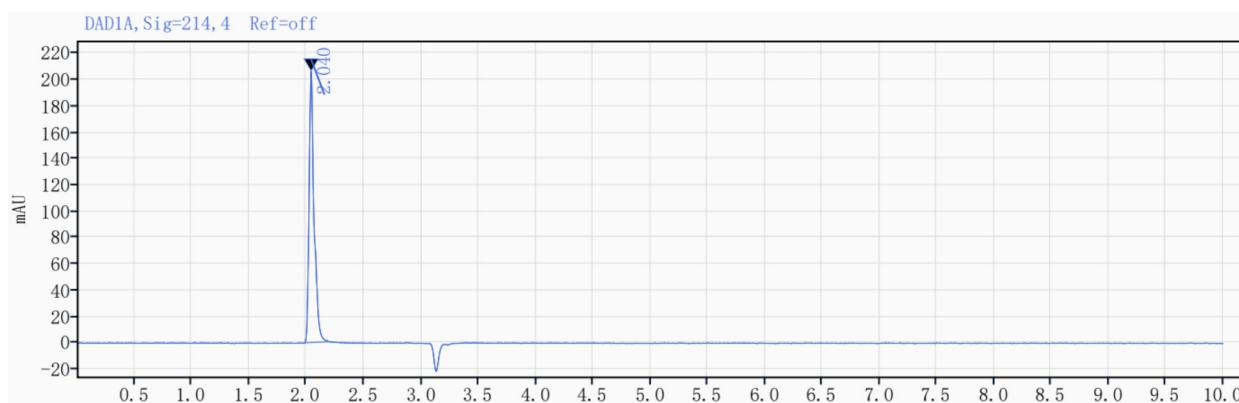

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	Blue to off-blue lyophilized powder	Blue to off-blue lyophilized powder (conforms)
Identification (Retention Time)	HPLC	±0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	≥ 99.0%	99.88%
Net Peptide Quantity	HPLC	50mg	52.27 mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by: 
Matt C.
Head of Quality Control