




Certificate of Analysis (CoA)

Product:	BPC157, TB500 and GHK-Cu (Glow)
Quantity:	5mg / 5mg / 20mg
Batch/Lot No.:	GL05-03-814-f470
Date of Analysis:	28 Nov 2025
Instrument:	Agilent 1260 HPLC and Thermo (MK3)

Quality Control

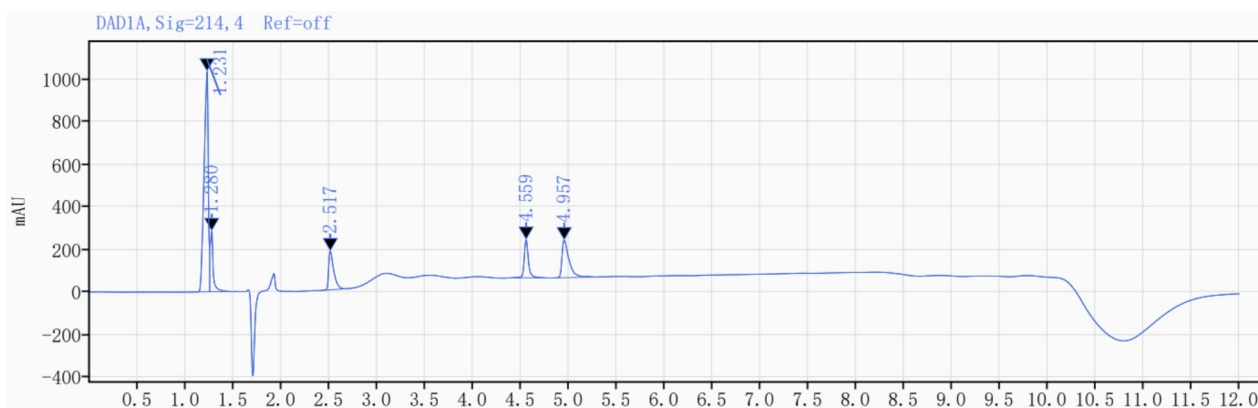

Test Parameter	Method	Specification	Result
Identification (Retention Time)	Visual inspection	Blue to off-Blue lyophilized powder	Blue to off-Blue lyophilized powder (conforms)
Identification (Retention Time)	HPLC	±0.2 min of Standard	Conforms
Purity (by HPLC, % area)	HPLC	≥ 99.0%	99.05%
Net Peptide Quantity	HPLC	5mg / 5mg / 20mg	5.07mg / 5.01mg / 19.41mg
Endotoxin	LAL	≤ 0.5 EU/mg	Conforms

Authorized by:

Matt C.

Head of Quality Control